

Figure 08 | Curve calibration and rate limits

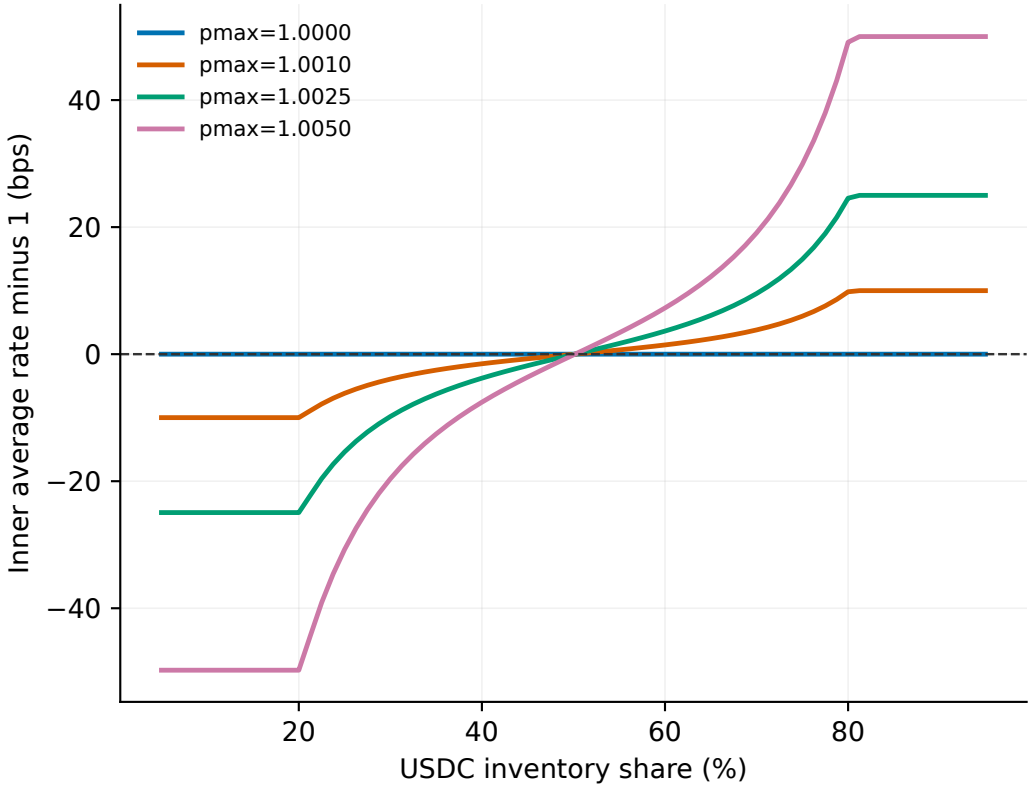

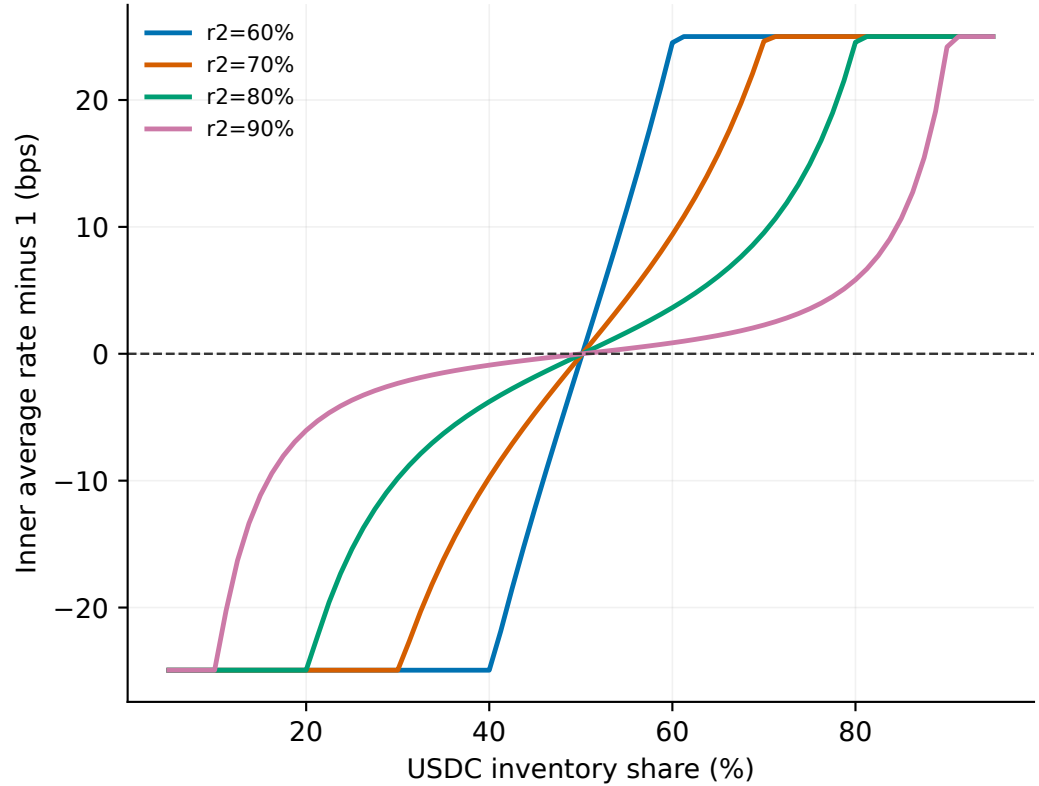

Base unless varied: q=100 USDT, T=30,000, f=50 bps, execution=$6.25; synthetic C/R; c37a0741